

## TECHNICAL DATA

# VPS220-R – Voltage Probe Set, 100:1, one red



## Product overview: VPS220-R – Voltage Probe Set, 100:1, one red

Double insulated voltage probe for ScopeMeter 190 series.

### Each probe set includes:

- 600 V CAT III / 1000 V CAT II rated 100:1 Voltage Probe
- Hook Clip for Probe Tip
- Ground Lead with Mini Alligator
- Insulation Sleeve
- 30 V CAT II rated Ground Spring for Probe Tip


### Specification:

- Attenuation: 100:1
- Bandwidth: 200 MHz
- Max. Input Voltage 1000 V CAT II or 600 V CAT III
- Max. Voltage to ground: 1000 V CAT II or 600 V CAT III per IEC / EN61010-031
- Input Resistance: 100 M $\Omega$
- Input Capacitance: 4.6 pF
- Compensation range: 10 to 25 pF
- Cable Length: 1.2 m

## Specifications: VPS220-R – Voltage Probe Set, 100:1, one red

Specification	
Attenuation	100:1
Bandwidth	200 MHz
Max. input voltage	1000 V CAT II or 600 V CAT III
Max. voltage to ground	1000 V CAT II or 600 V CAT III per IEC / EN61010-031
Input resistance	100 MΩ
Input capacitance	4.6 pF
Compensation range	10 to 25 pF
Cable length	1.2 m

## Ordering information

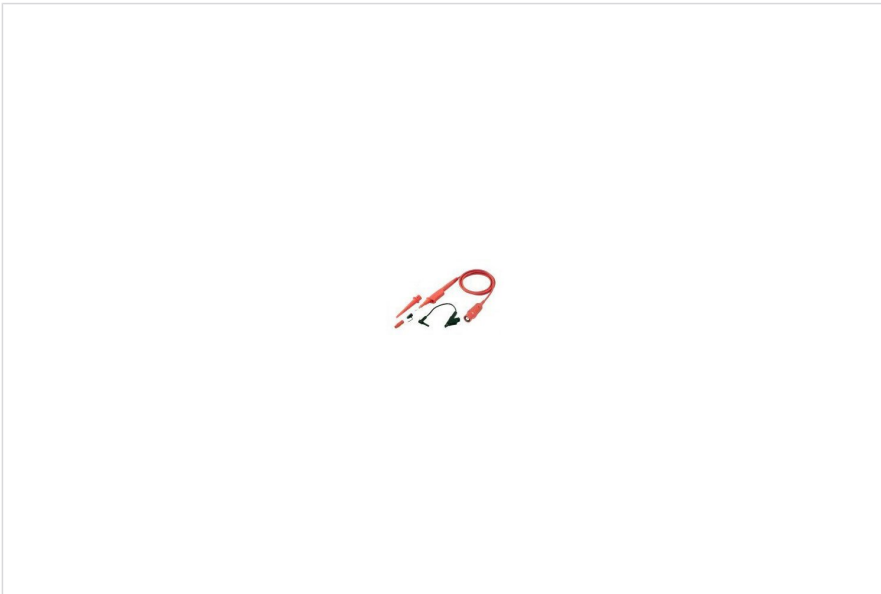

### **Fluke VPS220-R**

Voltage Probe Set, 100:1, One Red

---

Each probe set includes:

- 600 V CAT III / 1000 V CAT II rated 100:1 voltage probe
  - Hook clip for probe tip
  - Ground lead with mini alligator
  - Insulation sleeve
  - 30 V CAT II rated ground spring for probe tip
-

**Fluke.** *Keeping your world up and running.®*

**Fluke Corporation**

PO Box 9090, Everett, WA 98206 U.S.A.

**For more information call:**

In the U.S.A. (800) 443-5853

In Europe/M-East/Africa +31 (0)40 267 5100

In Canada (800)-36-FLUKE

From other countries +1 (425) 446-5500

**Fluke Electronics (Malaysia) Sdn Bhd**

Suite D-3A-4, Block D

SouthGage Commercial Centre, No2

Jalan Dua Off Jln Chan Sow Lin

55200 KL

Malaysia

Email: [info.asean@fluke.com](mailto:info.asean@fluke.com)

[www.fluke.com/my](http://www.fluke.com/my)

©2021 Fluke Corporation. Specifications subject to change without notice.

11/2021

**Modification of this document is not permitted without written permission from Fluke Corporation.**