


Data teknis

Fluke BHT190 Break-Out Adapters for Industrial Bus Connections

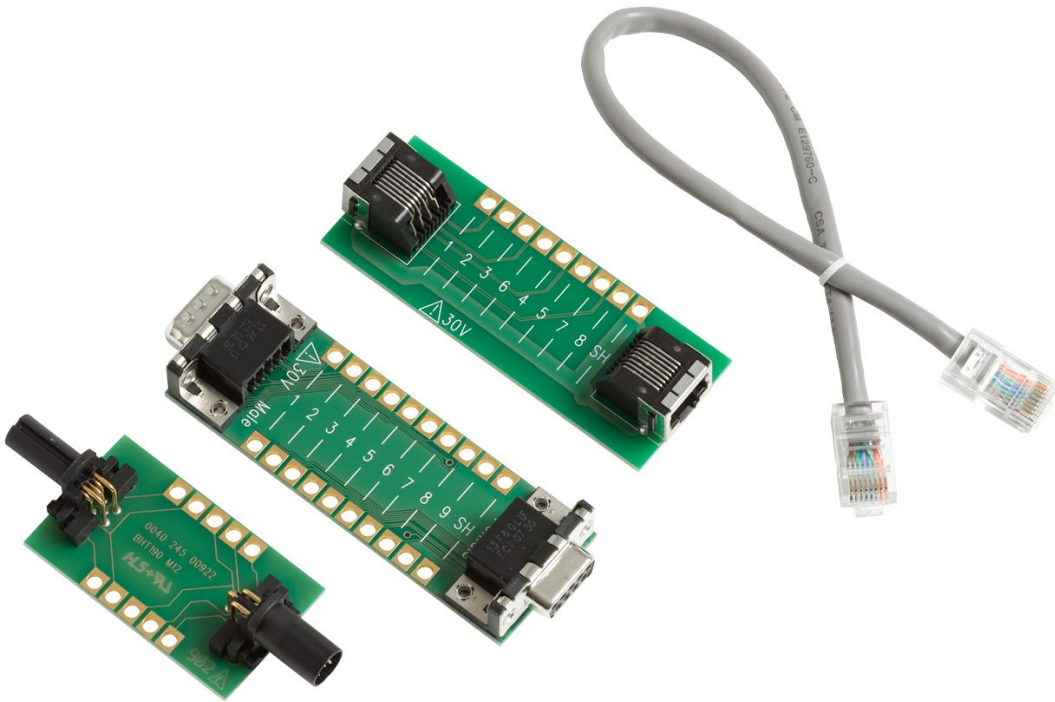

Fitur utama

Set contains:

- Break-out adapter DB-9, male-to-female. Gives access to pins 1 thru 9 and shield.
- Break-out adapter M12, with cables, male-to-female. Gives access to pins 1 thru 5.
- Break-out adapter RJ-45, female-to-female with patchcable (patchcable not shown on photo). Gives access to pins 1 thru 8 and shield.

Ikhtisar Produk: Fluke BHT190 Break-Out Adapters for Industrial Bus Connections

Set of break-out adapters for the three most common industrial bus connection systems M12, DB-9 and RJ-45. Each board works as a straight-through connection for the bus cable and gives access to the individual wires and pins of the connector system for hooking up probes.


Spesifikasi: Fluke BHT190 Break-Out Adapters for Industrial Bus

Connections

Specifications

Max. voltage	30 V rms, 42 V peak, between any connection and between connections and ground.
--------------	---

Model

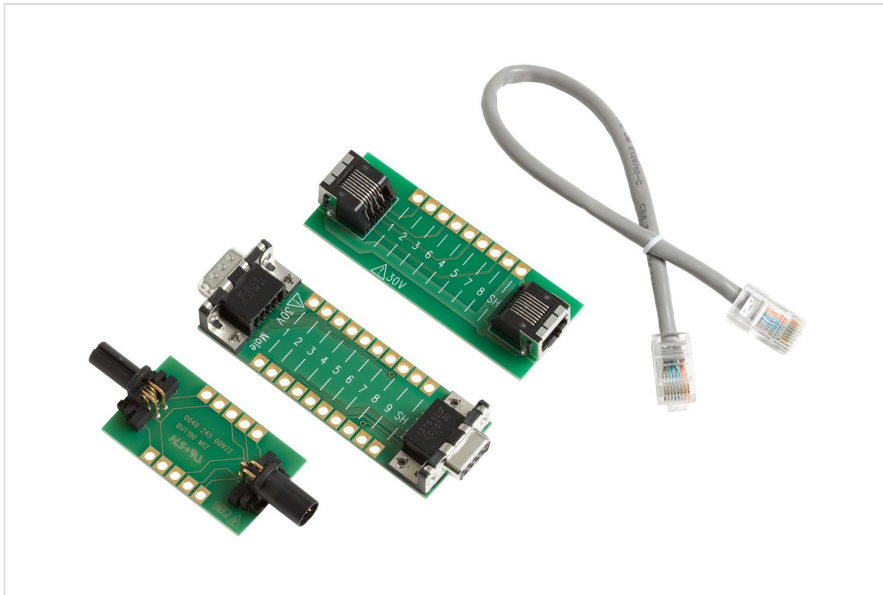

Fluke BHT190

Set contains:

- Break-out adapter DB-9, male-to-female. Gives access to pins 1 thru 9 and shield
 - Break-out adapter M12, with cables, male-to-female. Gives access to pins 1 thru 5
 - Break-out adapter RJ-45, female-to-female with patchcable (patchcable not shown on photo). Gives access to pins 1 thru 8 and shield
-

Fluke. *Memastikan aktivitas Anda terus berjalan dan beroperasi.*

Fluke Corporation

PO Box 9090, Everett, WA 98206 U.S.A.

For more information call:

In the U.S.A. (800) 443-5853

In Europe/M-East/Africa

+31 (0)40 267 5100

In Canada (800)-36-FLUKE

From other countries +1 (425) 446-5500

www.fluke.com

BUT. FLUKE SOUTH EAST ASIA PTE LTD

Menera Satu Sentra Kelapa Gading #06-05

Jl. Bulevar Kelapa Gading Kav. LA# No. 1

Summarecon Kelapa Gading

Jakarta Utara 14240

Indonesia

Tel: +62 21 2938 5922

Email: info.asean@fluke.com

www.fluke.com/id

©2021 Fluke Corporation. Specifications subject to change without notice.

12/2021

Modification of this document is not permitted without written permission from Fluke Corporation.